




PatellarTape System™

For Patellar Tendon
Reconstruction



Why PatellarTape System?

- Provides excellent intrinsic strength and allows early mobilisation.
- The use of metalwork and wire cerclage is unnecessary and the associated high complication rate and problems of secondary removal are thus avoided.
- The implant carries none of the risks or availability problems of allograft.
- There is no donor site morbidity as encountered with autograft.
- It is a straightforward technique with a low complication rate.
- The open weave structure of the implant acts as a scaffold that encourages tissue ingrowth.

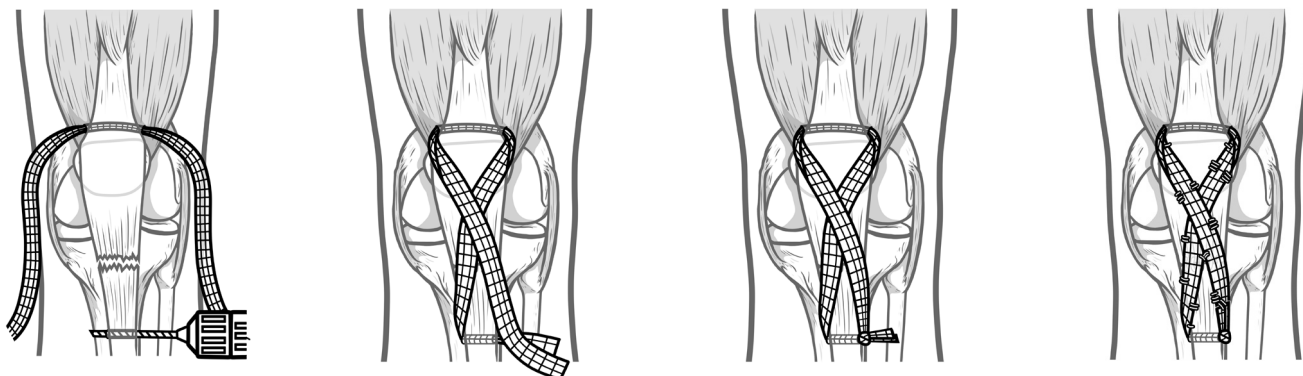

The information above **MUST NOT** be used to perform the surgical procedure.
Always refer to the Instructions for Use LAB 248 which contains detailed information and essential warnings and precautions.

Ordering Information

102-1062 **PatellarTape System™**, includes:

Poly-Tape, 30 mm x 800 mm (supplied sterile)

Packaged with the following disposables:

Malleable probe with eye, stainless steel, 20 cm (supplied sterile)

Rigid probe with eye, stainless steel, 20 cm (supplied sterile)

Drill bit, plain shank to fit Jacobs Chuck, 4.5 mm diameter (supplied sterile)



Get Involved

At Xiros we are constantly striving to improve outcomes for patients, and we want to hear from you. Help us create the future of sports medicine and share your opinions and expertise with us at: www.xiros.co.uk

Developed and manufactured by

Xiros™ Ltd

Springfield House, Whitehouse Lane, Leeds LS19 7UE

Tel. +44 (0) 113 238 7202 Fax. +44 (0) 113 238 7201

enquiries@xiros.co.uk

www.xiros.co.uk

Xiros Limited, registered in England No. 1664824.

Xiros and **PatellarTape System** are trademarks of Xiros.
All rights reserved. © Xiros™ 2023. Worldwide patents and patents pending.

LABAU 268 4.00

Distributed in Australia & New Zealand by:



Tel: + 61 (2) 9316 6665

Email: info@neosurgical.com.au